



EC-Type Examination Certificate

Measuring Instrument Directive

Certificate number: DK-0200-MI002-023

Issued by FORCE Certification A/S, Denmark
EC-notified body number 0200

In accordance with The Danish Safety Technology Authority's statutory order no. 436 of 16th May 2006 with later amendments which implements the Directive 2004/22/EC of the European Parliament and Council of March 31st, 2004 on measuring instruments (MID) and later amendments.

Issued to: **APATOR METRIX SA**
ul. Piaskowa 3
83-110 Tczew
Poland

Reference No.: 80.976-222/11

Type of instrument: Diaphragm Gas Meter with temperature conversion

Type designation: Uniflo G4S

Valid until: May 10, 2020

Number of pages: 6, including appendix

Date of issue: September 12, 2011

Revision: 1

This revision replaces the original certificate

Approved by

Hans Falster

Director

Processed by

Kurt Rasmussen

Certification Manager

The conformity markings may only be affixed to the above type approved equipment. The manufacturer's Declaration of Conformity may only be issued and the notified body identification number may only be affixed on the instrument when the production/product assessment module (D or F) of the Directive is fully complied with and controlled by a written inspection agreement with a notified body.

This EC-type examination certificate may not be reproduced except in full, without written permission by FORCE Certification A/S.



Appendix to EC-Type Examination Certificate Measuring Instrument Directive

Certificate no. DK-0200-MI002-023, Rev. 1.

Issued by FORCE Certification A/S, Denmark
EC-notified body number 0200

Revision history

Revision	Issue date	Changes
DK-0200-MI002-023 Rev. 1	2011-09-12	New references to current Danish statutory orders. New requirements for the verification MPEs. New photo for the mono-pipe model New description (text and drawing) of the main verification seal
DK-0200-MI002-023	2011-04-05	Original certificate

Applied standards and documents:

EN 1359:1998/A1:2006. Gas meters – Diaphragm gas meters.
EN 12405-1:2005/A1:2006. Gas meters – Conversion devices – Part 1. Volume conversion.
WELMEC Guide 7.2, Issue 4, may 2008. Software Guide (Measuring Instruments Directive 2004/22/EC).

The software fulfils the basic requirements for type P and specific requirements I2
The software fulfils the requirements for extension S and D.

The instrument shall correspond to the following specifications:

Type designation

Uniflo G4S

Description

Uniflo G4S is a diaphragm gas meter with electronic index. The gas meter converts the measured volume to volume at base condition (converted volume). The conversion is based on measured temperatures, a fixed set value of gas pressure and a fixed set conversion constant.

The meter is also available without temperature conversion. In that case the index is showing the corrected volume.

The mechanical measuring unit is mounted in a steel plate housing with either two-pipe or co-axial connections. The measuring unit's movements are transmitted via an optical scanning to the electronic index.

The calculator in the index registers the measured gas volume and calculates a volume corrected for the meter error determined during calibration. The calculator is fitted with a display showing the corrected volume, or the converted accumulated volume in m³ at base condition.

The meter may be verified at three different Q_{max} .

The meter is available with the following options:


- T temperature conversion
- M M-bus output
- V integrated valve
- R radio communication
- (blank) without any of the above options

Functional errors activate a warning triangle on the display.

The calculator is supplied with an IR communication interface which may be used for remote reading and coding of the calculator. Coding can only be made with a special configuration software after an electrical connection (jumper) has been mounted on the printed circuit board. The printed circuit board is protected by the metrologic cover, which again is secured by a verification seal. The software used in the calculator has version number 012400XX-YY, where XX and YY are of no significance to the measurement or in any other way may change the properties of the meter according to this EC-type examination certificate.

On start-up of the meter the index will show an abbreviated version of the software version number: 01 XX YY.

The meter is resistant to high ambient temperature and suitable for differential temperature and intermittent operation.

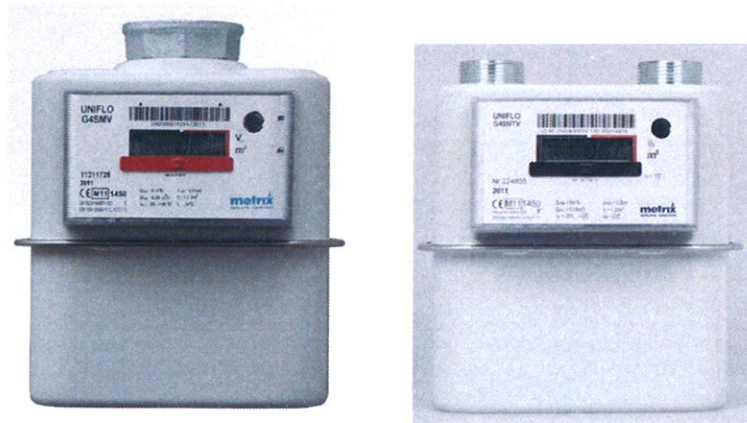

Technical documentation

FORCE Certification A/S File no. 80.976-085/09 (electronic index)

FORCE Certification A/S File no. 80.976-222/11 (gas meter)

Technical data

Instrument type:	Diaphragm gas meter with temperature conversion				
Accuracy class:	1,5				
Environment class:	M1, E2				
Climatic class:	-25°C to +55°C, condensing, closed outdoor location.				
Volume indication:	m ³ at base condition or corrected volume at actual conditions				
Maximum flow rate:	Q _{max}	2,5	4	6	m ³ /h
Minimum flow rate:	Q _{min}	0,016	0,025	0,04	m ³ /h
Transitional flow rate:	Q _t	0,25	0,4	0,6	m ³ /h
Overload flow rate:	Q _r	3,0	4,8	7,2	m ³ /h
Cyclic volume	V	1,2 dm ³			



Gas family:	Fuel gasses of 1 st , 2 nd and 3 rd family (EN 437:2003)	
Maximum pressure:	p_{max}	0,5 bar g
Gas temperature range:	t_m	-25 °C to +55 °C
Base gas temperature:	$T_{b,i}$	0 to 20 °C
Base pressure:	p_b	1013 mbar
Base volume:	V_b	0 – 99999.9999 m ³
Specified temperature:	t_{sp}	20 °C
Power supply	3 or 3.6 V Lithium battery, AA, double AA or C-cell, ER 6 / ER20 according to IEC 86-1, "Primary batteries"	

High ambient temperature resistant

The meter is supplied with different connections:

Two-pipe, with centre distance 110 to 250 mm, threads from 1/2" to 5/4"

Mono-pipe (coaxial) 2"

Software

Version no.: 012400XX-YY
01 is the version no. for the approved legal part of the software
2400 is the type no.
XX is the application no.
YY refers to the hardware.

Display: In the display is shown 01 XX YY on start-up
Checksum: Legal software ver. 01 has the checksum 10799
Main PCB 6024800-01-0001: For wired M-bus
6024801-01-0001: For option board

Verification

Errors

Maximum permissible errors (MPE) according to Directive 2004/22/EC of the European Parliament and Council of March 31st, 2004 on measuring instruments (MID), Annex MI-002.

Ambient temperature t_{am} : -25 °C to +55 °C

Maximum permissible errors

For t_{am} : +5 °C to +35 °C
 $\pm 3 \%$ for $Q_{min} \leq Q < Q_t$
 $\pm 1,5 \%$ for $Q_t \leq Q < Q_{max}$

The gas meter shall not exploit the MPEs or systematically favour any party.

If the meter indicates the converted volume an additional increase of 0,5 % to MPE is permitted for in the temperature interval 5 °C to 35 °C. Outside this temperature range an additional increase of 0,5 % is permitted in each interval of 10 °C.

Procedure

Verification is carried out at laboratory conditions. It is permitted to use air as verification gas. The verification is valid only for the display reading of converted volume V_b or corrected volume V_c .


Sealing

Verification sealing


The main verification seal is placed in the metrologic cover. The main verification seal locks the index to the meter body, and the front label to the index. The metrologic cover is sealed with the main verification seal, and a secondary seal. The main verification seal consists of two shaped letters "Mx" encircled in a serrated octagon.

Installation sealing

The transparent front cover is secured by two installation seals, one on each side of the index. The installation seals are small plastic caps which are pressed and locked into a hole in the cover and index. The seals are marked with the year of sealing.

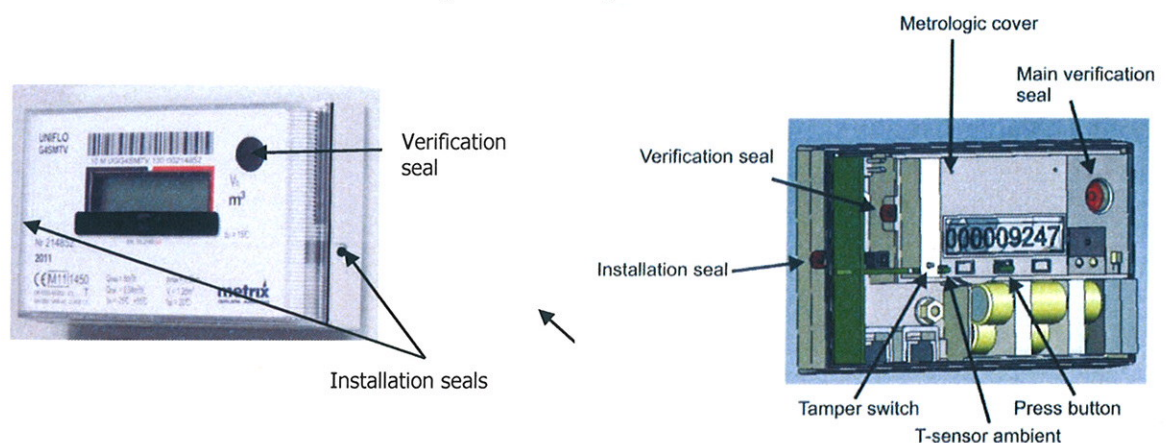

Labelling and inscriptions

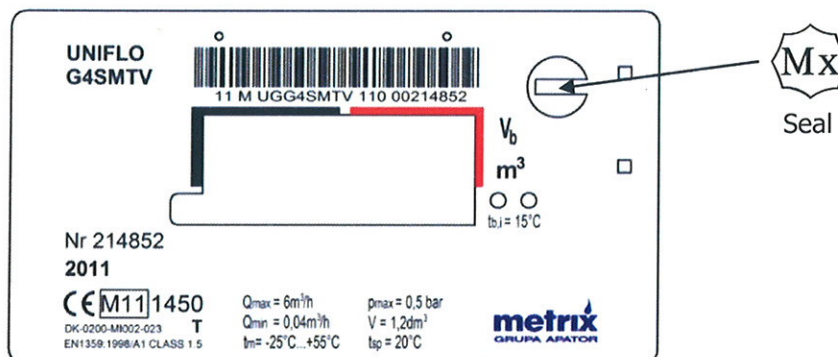

Conformity marking (CE + M + Year of affixing + NB no.)

EC-type examination certificate number

Manufacturer designation or logo

Type, production year and serial number

Applied European Standard : EN 1359:1998/A1:2006

Class : 1,5

Maximum flow rate: Q_{max} : 2,5 4 6 m³/h

Minimum flow rate: Q_{min} : 0,016 0,025 0,04 m³/h

Ambient and gas temperature: t_m : -25 °C ... +55 °C

Base gas temperature: t_{b,i} : 0 to 20 °C

Specified temperature: t_{sp} : 20 °C



Maximum working pressure:	p_{\max}	:	0,5 bar g
Volume:	V_b or V_c	:	m^3
Cyclic volume:	V	:	1,2 dm^3
High ambient temperature resistant		:	T

Accompanying information

Rated operating conditions not included on the label:

- Transitional flow rate: $Q_t = 0,1 Q_{\max}$
- Overload flow rate: $Q_r = 1,2 Q_{\max}$
- Climatic class: condensing, closed outdoor location
- Mechanical and electromagnetic environment classes: M1, E2
- Gas family: Fuel gasses of 1st, 2nd and 3rd family (EN 437:2003)
- Power supply: Lithium battery, 3 or 3.6 V DC
- Software version number: 012400XX-YY
- Legal software checksum: 10799

Suitable for significantly different ambient and gas temperatures.

Instructions for installation, maintenance, repairs, permissible adjustments

Instructions for correct operation and any special conditions of use